

# Foam Pad



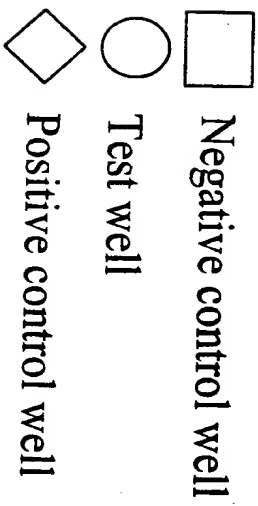


FIGURE 1

FIGURE 2

FIGURE 2

## Open Spectrophotometer on Palm

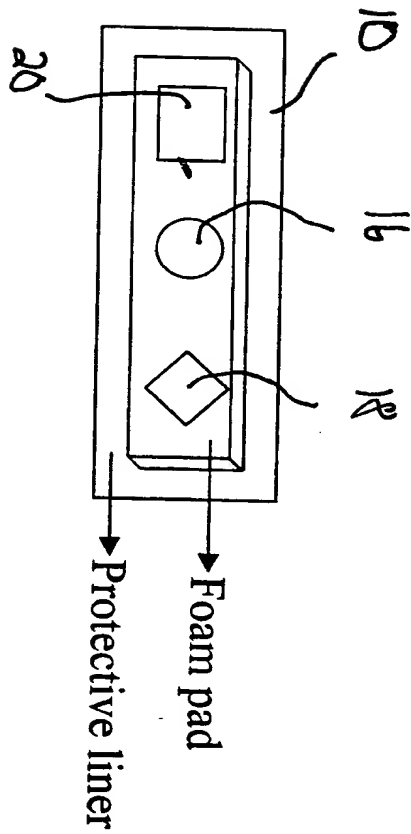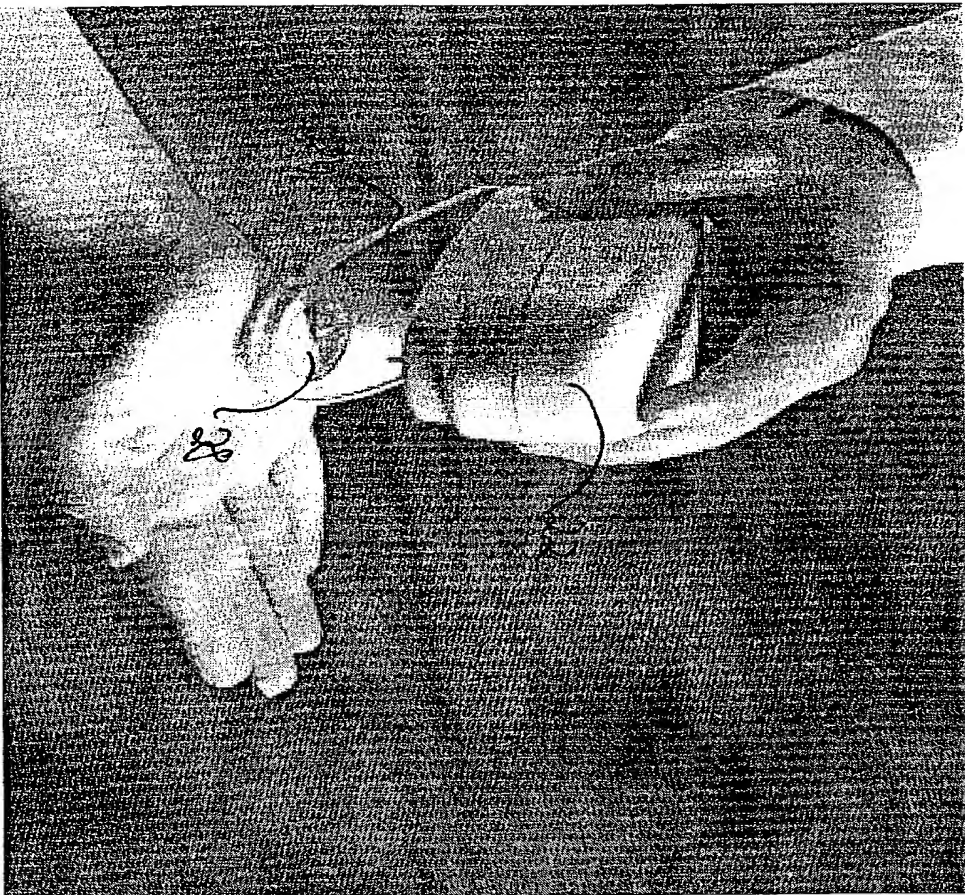


The spectrophotometer is placed on the foam pad on the palm at the end of the test such that the target window on the spectrophotometer aligns with the round center well on the foam pad.

FOIEBO 8020E860

FIGURE 3

## Closed Spectrophotometer on Palm

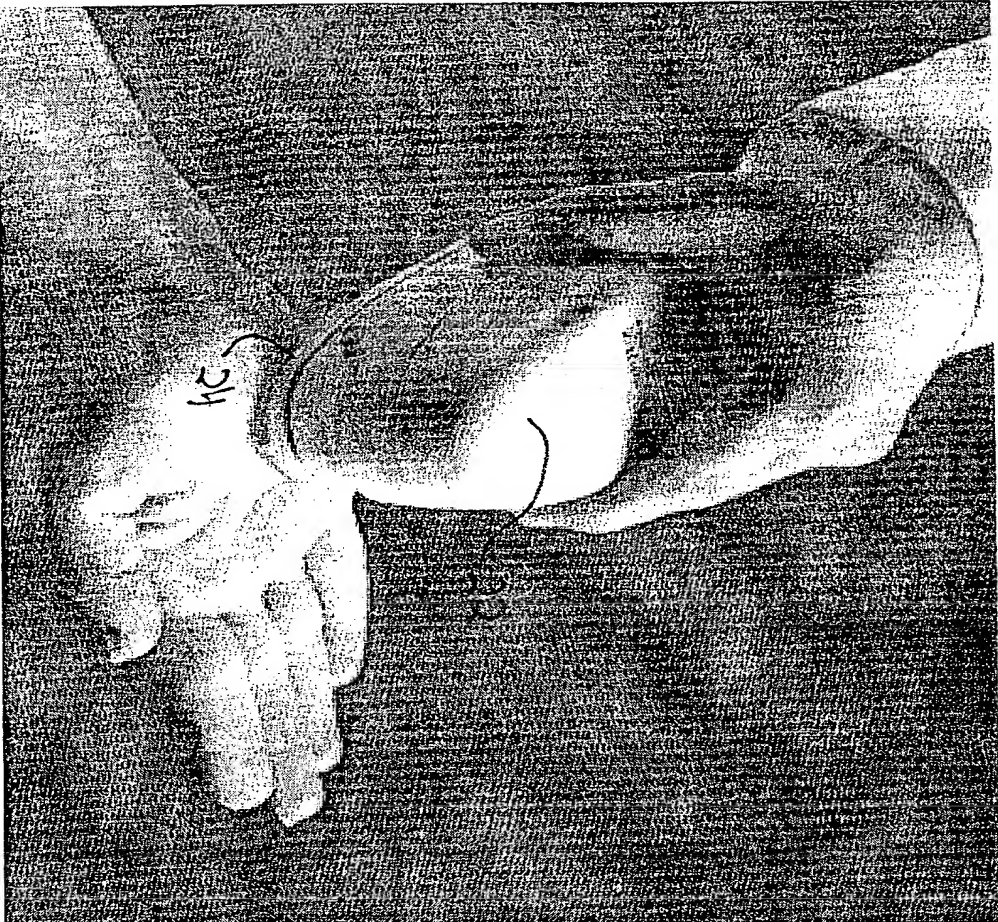

After proper positioning of the device, it is closed to activate the spectrophotometer. This results in measuring the patient's skin cholesterol (hue angle of the colour development in the test well).

09/03/03

WO 01/11359

PCT/CA00/00918

4/4

FIGURE 4

FIGURE 4

“Shoe” of Spectrophotometer

